



## PUD No. 1 of Chelan Co. TDG Monitors

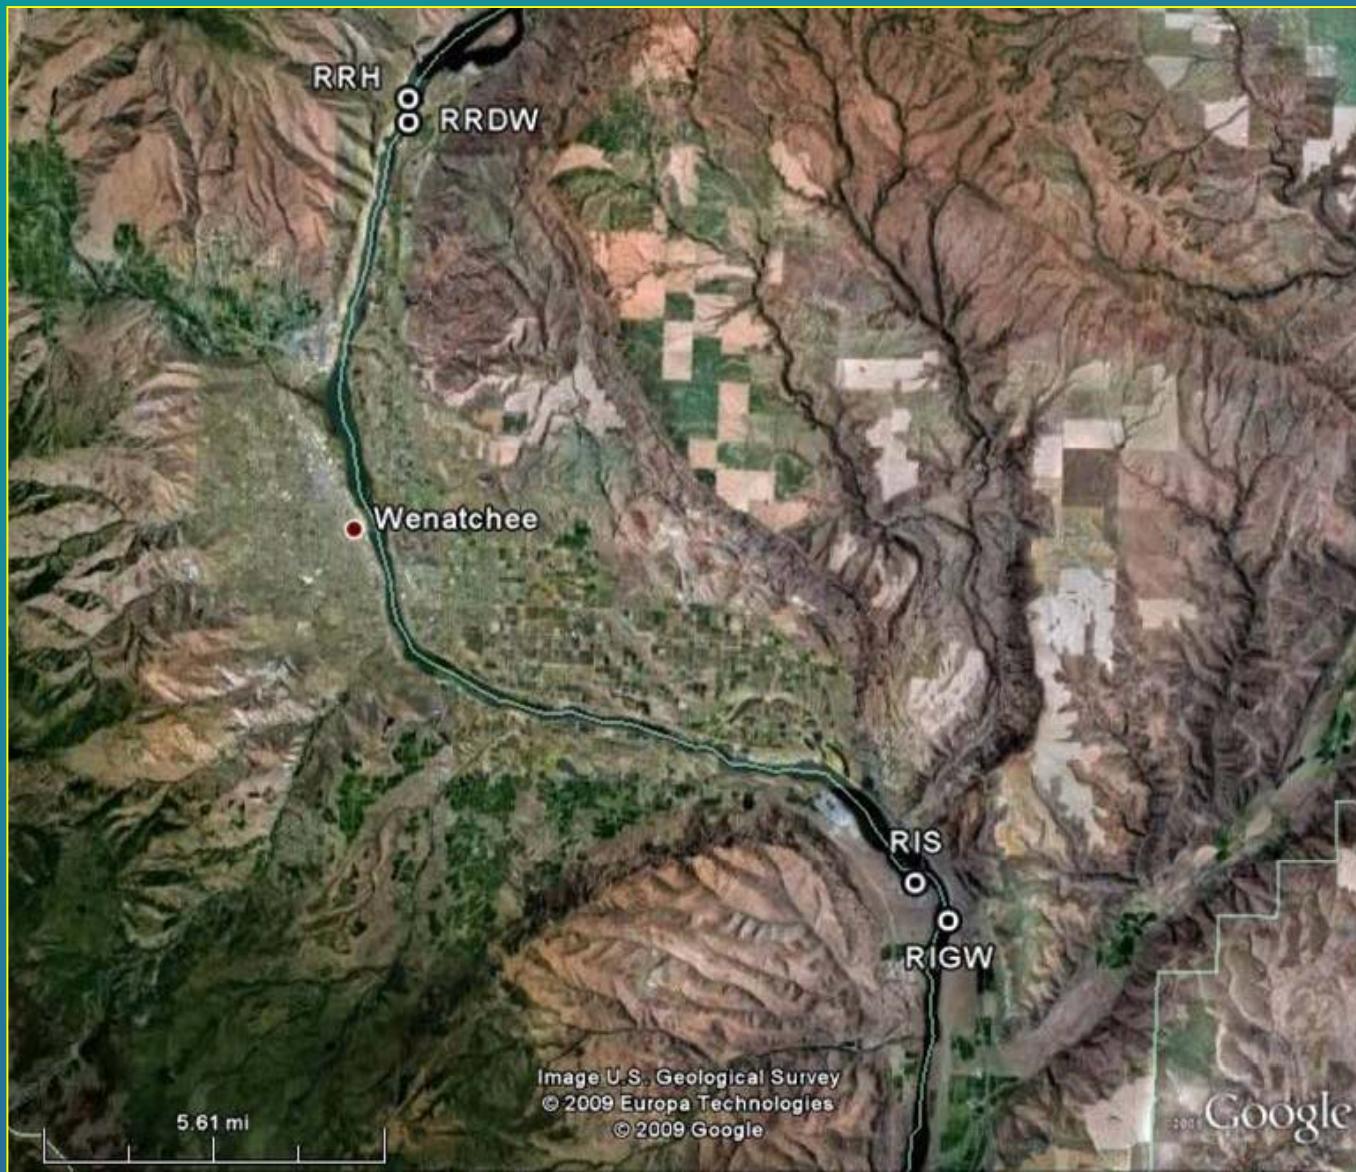

# CPUD 2010 Calibration Summary Box Plots

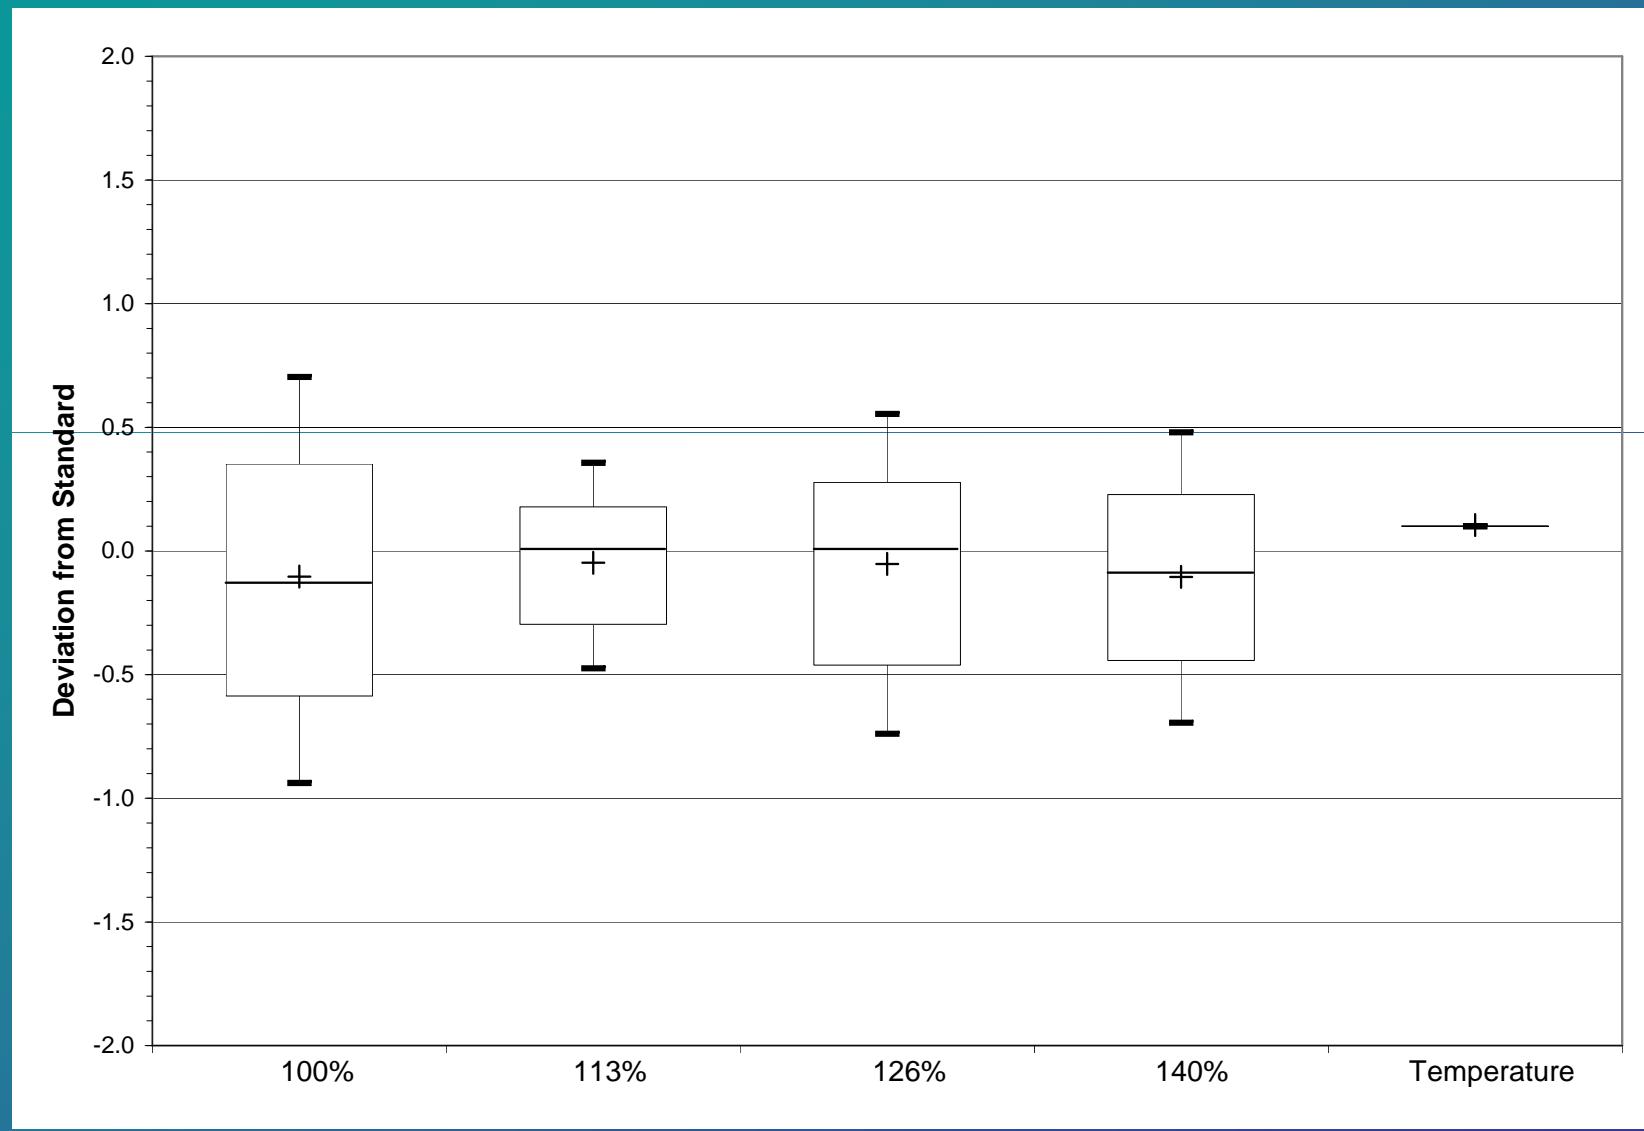

# PUD No. 1 of Chelan County 2010 Calibration Summaries

	Temperature (°C)	TDG Pressure (mmHg)			
		100%	113%	126%	140%
<b>Mean</b>	0.10	-0.10	-0.05	-0.05	-0.10
<b>Median</b>	0.10	-0.13	0.00	0.00	-0.10
<b>Standard Deviation</b>	0.07	0.20	0.17	0.16	0.15
<b>Variance</b>	0.00	0.04	0.03	0.03	0.02
<b>Minimum</b>	0.00	-0.54	-0.36	-0.42	-0.38
<b>Maximum</b>	0.20	0.40	0.36	0.32	0.29
<b>n</b>	22	22	22	22	22